


Injection Date: Fri, 18. Aug. 2023 Seq Line : 4
Sample Name : Cyanidin-3-o-rhamnoside chloride Location : 样品瓶 54
Acq Operator : DYH Inj. No. : 1
Inj. Vol. : 10 µl

Acq. Method : E:\Chem32\2\DATA\20230818\20230818-3 2023-08-18 17-4->
Analysis Method : D:\CHEM32\1\METHODS\Cyanidin-3-o-rhamnoside chloride.M
Last Changed : Fri, 1. Jul. 2022, 01:03:24 pm

Mobile Phase A: Methanol 30
Mobile Phase B: (0.25mol/L Tartaric acid)Water 70
Flow rate : 0.8ml/min
Temperature : 30°C
Column :Kromasil C18 250*4.6mm 5µm 100A
Sample Concentration: 0.5mg/ml mobile phase
Injection volume: 10µl

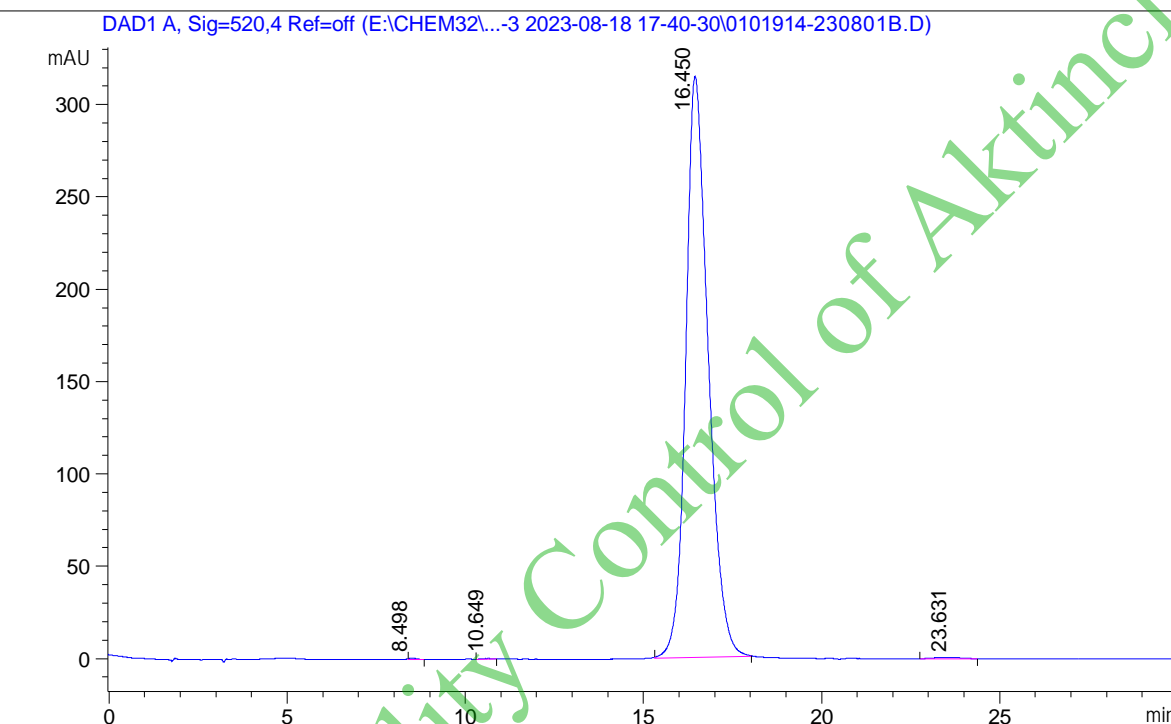

Customized Report: 简短报告

Sorted By Signal
Calib. Data Modified : Fri, 14. Oct. 2005,03:14:45 pm
Multiplier : 1.000000
Dilution : 1.000000
Uncalibrated Peaks : not reported

Signal 1: DAD1 A, Sig=520,4 Ref=off

Peak #	RT [min]	Type	Width [min]	Height	Area	Area %
1	8.498	MM	0.243	0.650	9.492	0.069
2	10.649	MM	0.307	0.341	6.277	0.045
3	16.450	BB	0.647	314.614	1.379e4	99.588
4	23.631	MM	0.905	0.759	41.234	0.298

=====

*** End of Report ***

Quality Control of Aktinchem